



4.5 mm TPLO System

VAR-4045S



Pic.	Item Number	Qty.	Description
1	VAR-13303-3.0		Osteotomy Guide Pin, 3.0 mm
2	VAR-8967K		K-Wire, 0.092 in (2.3 mm)
3	VAR-8941K		K-Wire, 0.062 in (1.57 mm)
4	VAR-8826M		Mini Mallet, 7 in
5	VAR-13203-05		Small Osteotome, 5 mm
6	VAR-13210		Low Profile Hohmann Retractor
7	VAR-4000TPS		TPLO Tissue Protector, standard
8	VAR-4045-01		Locking Plate Holder, 4.5 mm
9	VAR-4045S-R		TPLO Plate, 4.5 mm, standard, right
10	VAR-4045S-L		TPLO Plate, 4.5 mm, standard, left

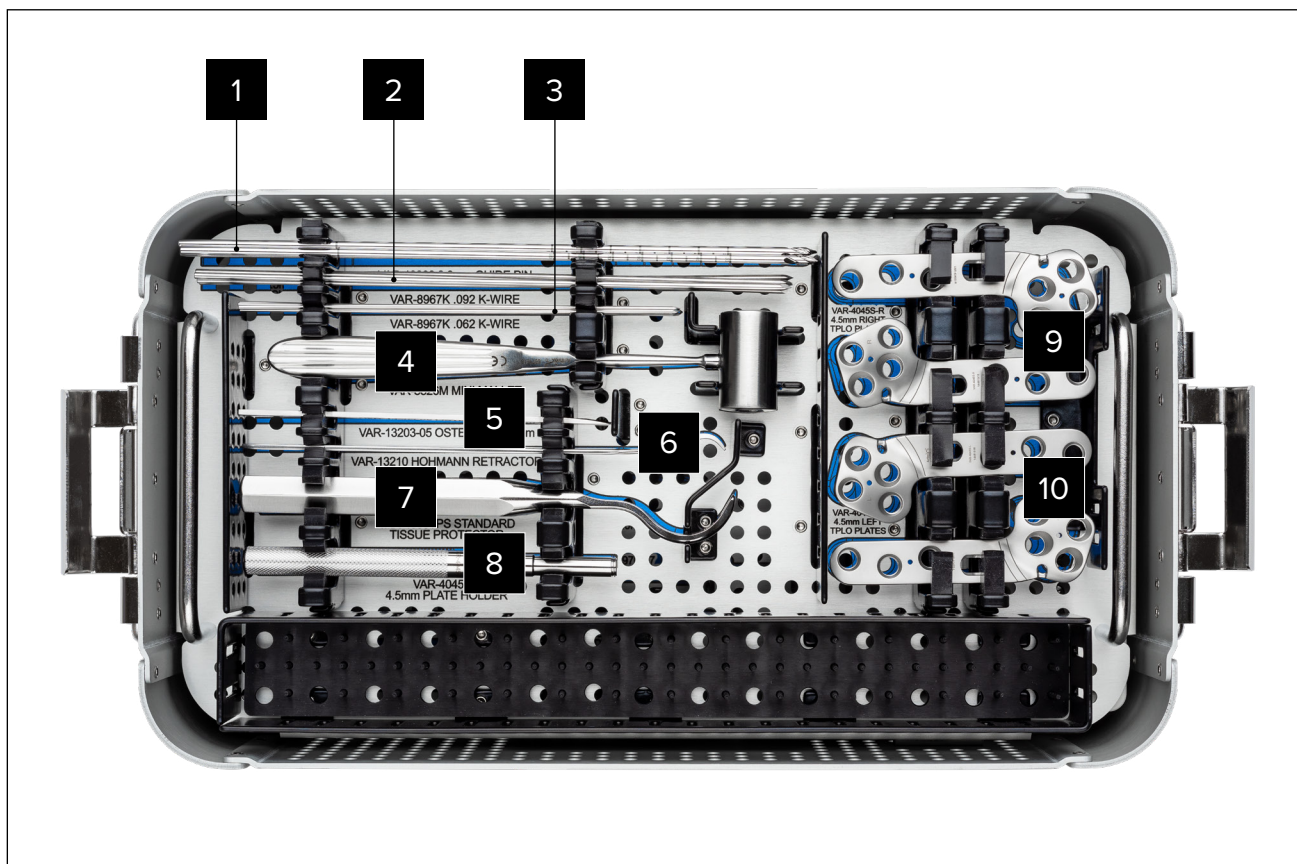

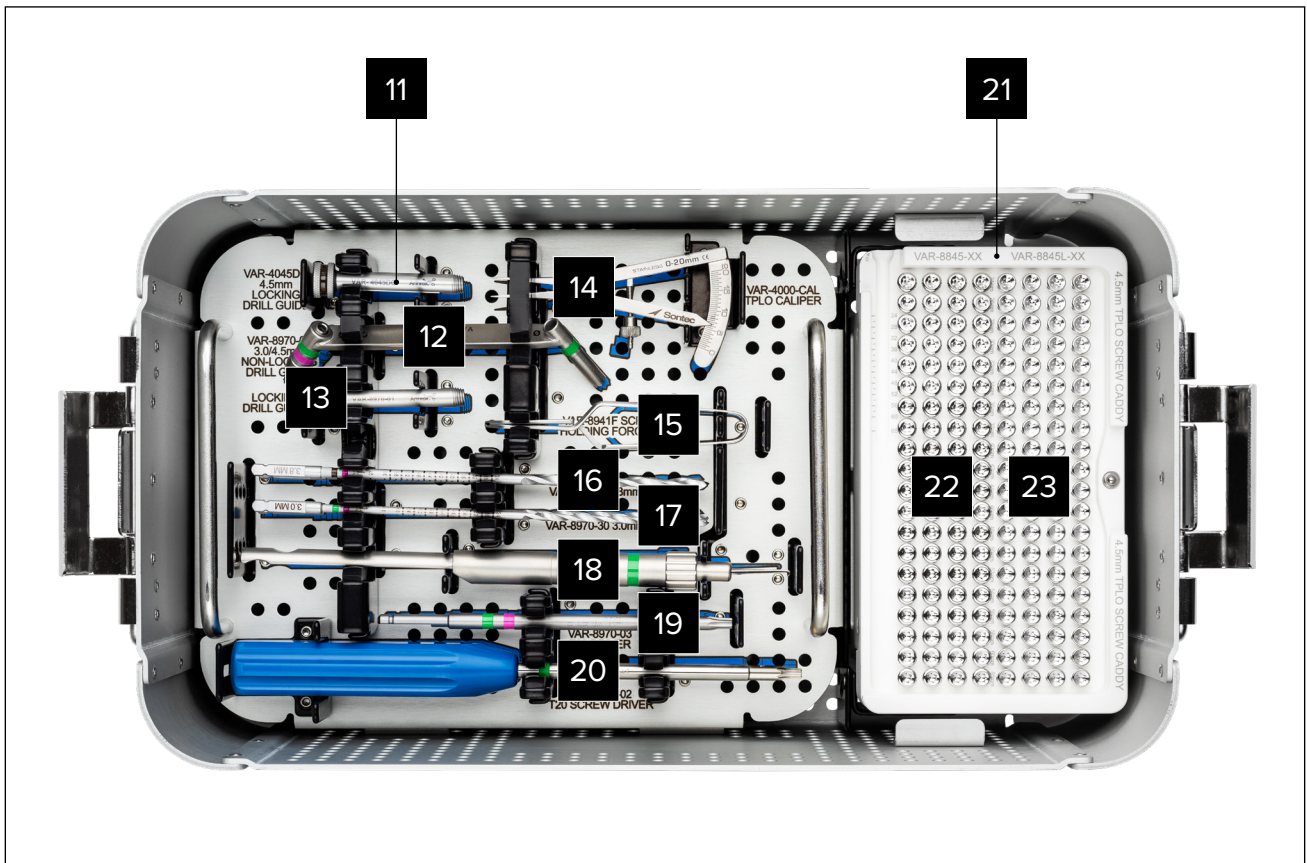

Pic.	Item Number	Qty.	Description
11	VAR-4045DG		Locking Drill Guide, 4.5 mm, 3.8 mm bit
12	VAR-8970-02		Nonlocking Drill Guide, 4.5 mm
13	VAR-8970-01		Locking Drill Guide, 4.5 mm, 3.0 mm bit
14	VAR-4000-CAL		TPLO Caliper
15	VAR-8941F		Screw Holding Forceps
16	VAR-4045D		Drill Bit, 3.8 mm
17	VAR-8970-30		Drill Bit, 3.0 mm
18	VAR-8970-07		Depth Device, 4.5 mm/5.5 mm
19	VAR-8970-03		T20 Driver
20	VAR-4045-02		T20 Screwdriver
21	VAR-4045SC-01		TPLO Screw Caddy, 4.5 mm
22	VAR-8845-24 to -65		Low Profile Cortical Screw, stainless steel, 4.5 mm x 24 mm to 60 mm + 65 mm
23	VAR-8845L-24 to -65		Low Profile Locking Screw, stainless steel, 4.5 mm x 24 mm to 60 mm + 65 mm



4.5 mm TPL0 System

VAR-4045S

Date of Surgery:

Surgeon Name:

Account:

Representative Contact Information:

Set Total:

Miscellaneous Notes:

To obtain a copy of a product's directions for use (DFU), which includes sterilization instructions, please visit our website at www.arthrex.com/edfu or contact your local representative.

